

Certificati Mascherine consegne dal 5/05/2020



ZERTIFIKAT ◆ CERTIFICATE ◆ 認証証書 ◆ CERTIFICADO ◆ CERTIFICAT

TMC
Access to global market

Declaration of Conformity

Certificate No.: TMC200317103-S

Applicant/
Address: **Zhongshan Dongfeng Huangshang Electronic Factory**
2F, No. 172, Dongfeng Da Dao Nan, An Le Cun, Dongfeng Town, Zhongshan City

Manufacturer/
Address: **Zhongshan Dongfeng Huangshang Electronic Factory**
2F, No. 172, Dongfeng Da Dao Nan, An Le Cun, Dongfeng Town, Zhongshan City

Product Name: **Protective Respirator**

Trade Name: N/A

Model/Item Number: GM700

Rated: -

Classification: FFP2

Date and
Number of Test Report: March 19, 2020
TMC200317103-S

EC-directive: PPE Directive (EU) 2016/425

Test Standard: EN149:2001+A1:2009

Conclusion
This Declaration of PPE Compliance has been granted to applicant based on the results of tests, performed by Laboratory of TMC Testing Services (Shenzhen) Co., Ltd. on sample of the above-mentioned product in accordance with the provisions of the relevant specific standards and the PPE Directive (EU) 2016/425. It is possible to use CE marking to demonstrate the compliance with this Directive.

Place and date of issue: Shenzhen, March 19, 2020
TMC Testing Services (Shenzhen) Co., Ltd.
1st Floor, Block A1, Zone A, Xinshidai Gongrong Industrial Park, No. 2,
Shihuan Road, Shiyan Street, Baoan District, Shenzhen, China
Tel: +86-755- 86642861
Email: cert@tmc-lab.com
Http://www.tmc-lab.com



TMC

Certificati Mascherine consegne dal 5/05/2020




检验检测报告

防伪查询网址: www.gttc.net.cn
防伪码: NLYM-5963-04
共3页 第1页



No.: 200021909




委托单位	中山市东凤镇皇尚电子 地址: 中山市东凤镇安家村东风大道南172号2楼		
客户认定信息	民用防护口罩 40个 颜色: 本白		
检验性质	委托检测	样品受理/测试开始日期	2020-02-24
判定依据	GB 2626-2006 (呼吸防护用品 自吸过滤式防颗粒物呼吸器)		
综合检验结论			
检验检测结果	检验检测项目	判定依据	判定
	NaCl颗粒物过滤效率	GB 2626-2006	符合
	吸气阻力	GB 2626-2006	符合
	呼气阻力	GB 2626-2006	符合
备注	<p>本报告中检验检测项目均在相应标准规定的环境下进行(有注明的除外) 复印件, 副本未重新加盖报告书确认章无效。 本报告检验检测地址为广州市番禺区市桥江涌1号。</p>		



签发: 方明 工程师

样品图片

No.: 200021909
共3页 第2页

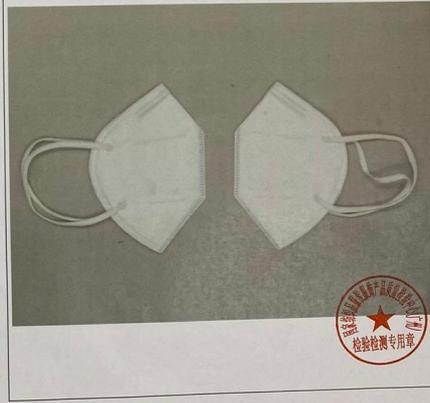



总部: 广州市番禺区市桥江涌1号
花都实验室: 广州市花都区新街镇康村河滨西路1号

电话: 020-61945968/61945969
电话: 020-37721161

总部: 广州市番禺区市桥江涌1号
花都实验室: 广州市花都区新街镇康村河滨西路1号

电话: 020-61945968/61945969
电话: 020-37721161



TEST REPORT 检验检测报告

NO. 200021909
共3页 第3页

3. 对委托送检、国家质量监督抽查检验结果有异议的监测, 其他监督检验向下达任务机关提出。
4. 检测结果仅对所检样品有效。
5. 未取得资质认定的项目, 仅作为科研、教学或内部。
6. 报告书涂改无效。

检验检测报告附页

No.: 200021909
共3页 第3页

检验检测项目 [计量单位] [样品识别]	测试方法	标准值及公差	检验检测结果	判定	备注
● NaCl颗粒物过滤效率	GB 2626-2006 6.3 空气流量: 85L/min 气溶胶颗粒: NaCl 气溶胶浓度: 10mg/m ³ 温度: 23.0°C 相对湿度: 35.8%	过滤效率(%) ≥95.0 (X95)	未处理样品 1# 99.981 2# 99.869 3# 99.769 4# 99.892 5# 99.881 6# 99.802 7# 99.804 8# 99.815 9# 99.790 10# 99.854 温度预处理后样品 1# 99.683 2# 99.857 3# 99.592 4# 99.811 5# 99.670	符合	
● 吸气阻力(Pa)	GB 2626-2006 6.5	≤350	未处理样品 1# 86.3 2# 83.9 温度预处理后样品 1# 83.9 2# 84.7	符合	
● 呼气阻力(Pa)	GB 2626-2006 6.6	≤250	未处理样品 1# 62.1 2# 63.3 温度预处理后样品 1# 55.5 2# 58.7	符合	
备 注	(本栏空白)				



总部: 广州市番禺区市桥江涌1号
花都实验室: 广州市花都区新街镇康村河滨西路1号

电话: 020-61945968/61945969
电话: 020-37721161

总部: 广州市番禺区市桥江涌1号
花都实验室: 广州市花都区新街镇康村河滨西路1号

电话: 020-61945968/61945969
电话: 020-37721161

